


Filename: Randolph_libs - 2021-11-16 - 14.02.12.D1000

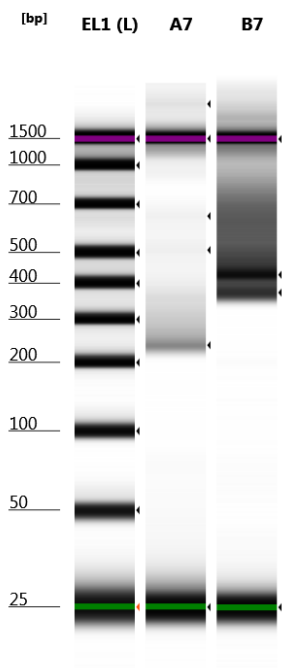


Default image (Contrast 129%)

Sample Info

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
EL1	20.3	Electronic Ladder		Ladder
A7	1.31	T		
B7	6.47	16s		

EL1: Electronic Ladder

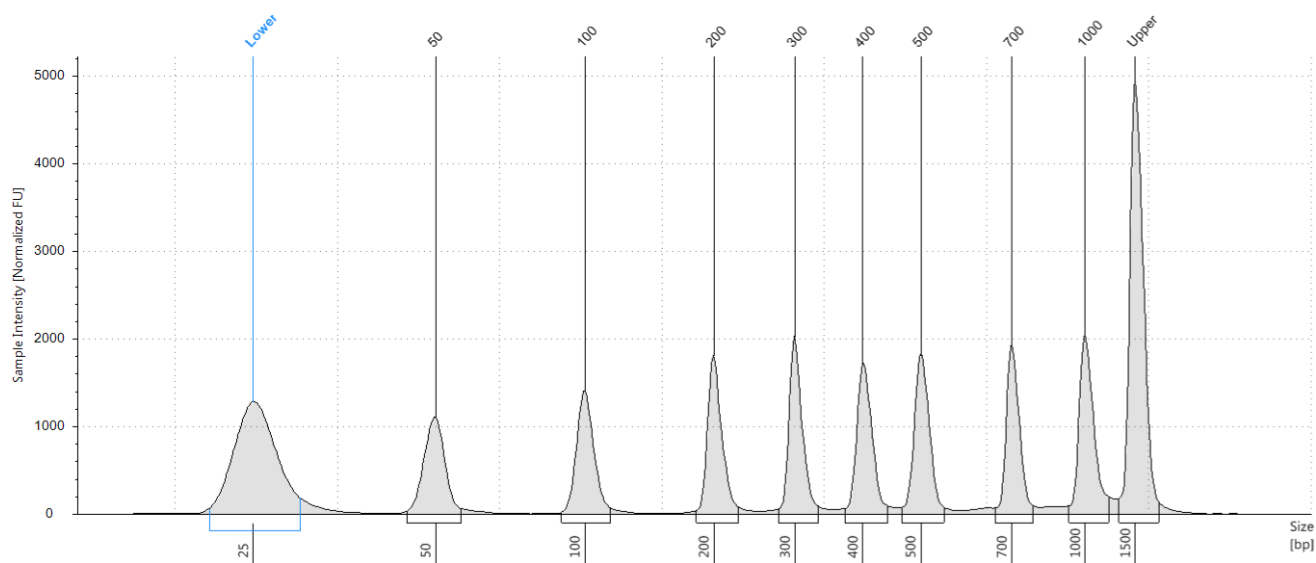


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
EL1	20.3	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.22	-	321	-		Lower Marker
50	2.25	-	69.3	11.11		
100	2.37	-	36.5	11.71		
200	2.47	-	19.0	12.20		
300	2.55	-	13.1	12.56		
400	2.57	-	9.87	12.66		
500	2.71	-	8.33	13.36		
700	2.46	-	5.41	12.15		
1000	2.89	-	4.44	14.25		
1500	6.50	6.50	6.67	-		Upper Marker

A7: T

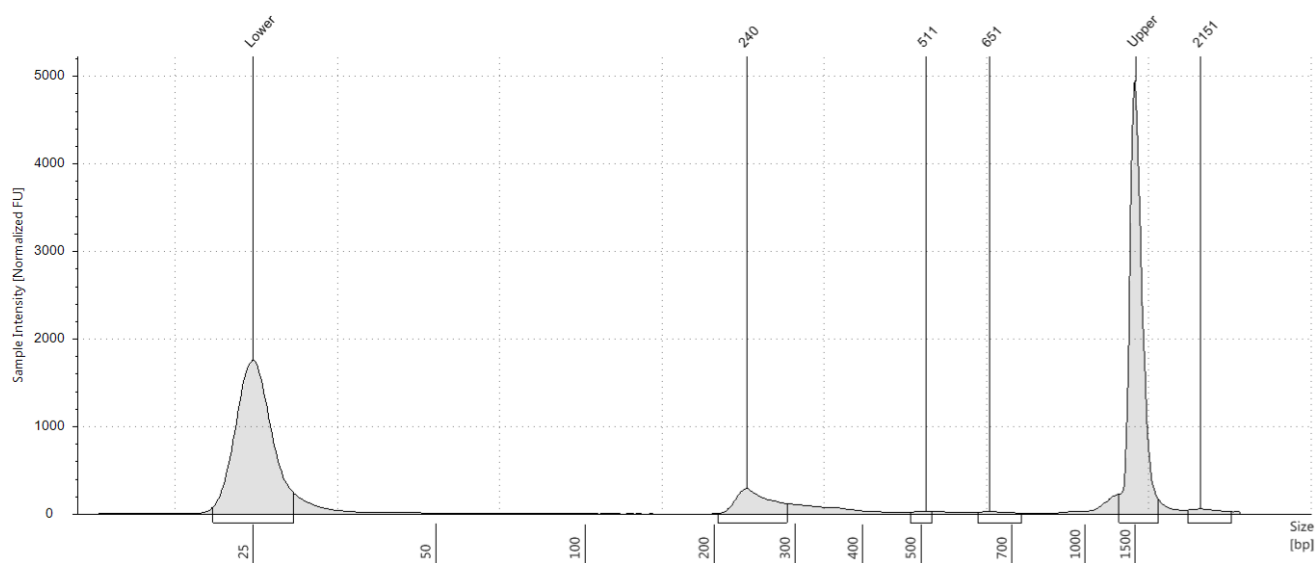


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A7	1.31	T		

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.70	-	412	-		Lower Marker
240	1.01	-	6.48	77.24		
511	0.0530	-	0.160	4.04		
651	0.0740	-	0.175	5.65		
1500	6.50	6.50	6.67	-		Upper Marker
2151	0.171	-	0.122	13.06		

B7: 16s

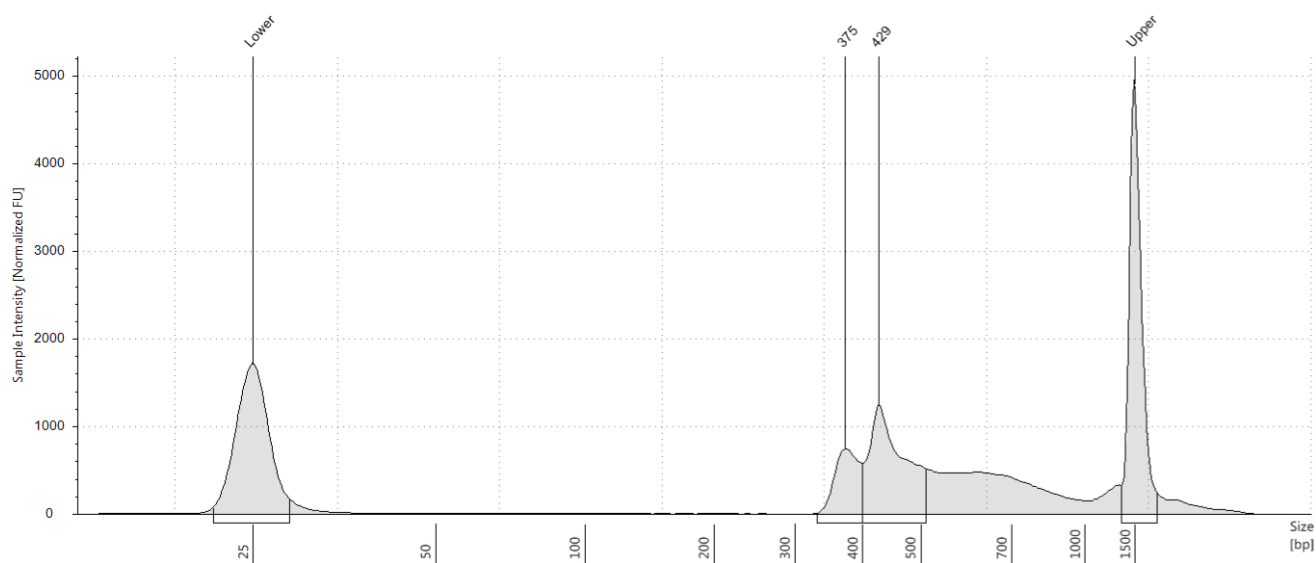

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B7	6.47	16s		

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.12	-	377	-		Lower Marker
375	1.94	-	7.94	29.94		
429	4.54	-	16.3	70.06		
1500	6.50	6.50	6.67	-		Upper Marker